




Mobile Shower Commode Chairs

Raz-AT (Z300)

User and Dealer Manual

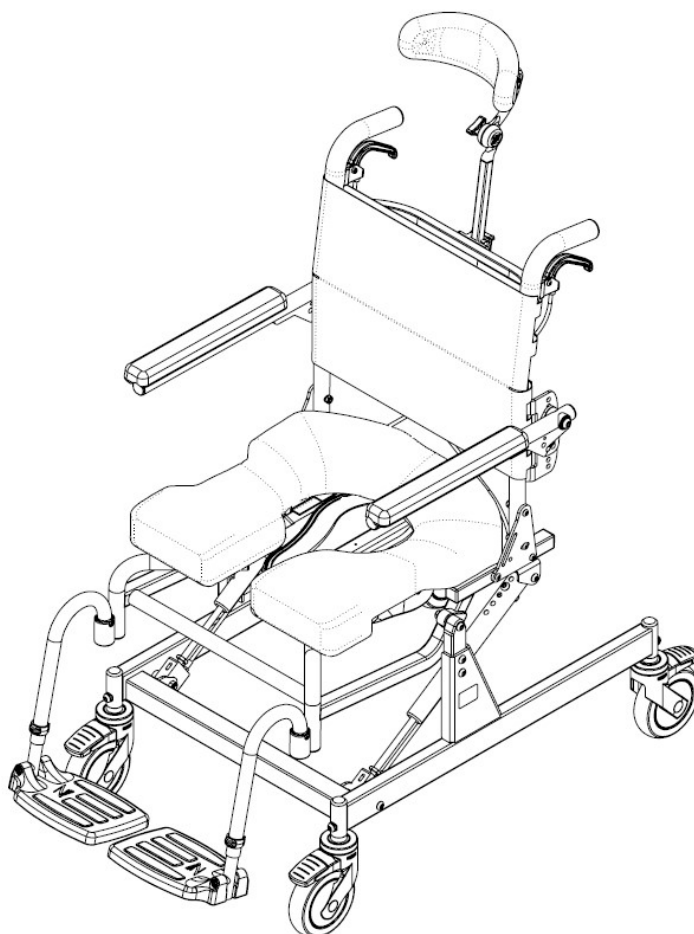

EC REP

Advena Ltd. Tower Business Center
2nd Flr, Tower Street
Swatar, BKR 4013 Malta

UKRP

Advena Ltd. Pure Offices, Plato Close
Warwick, CV34 6WE UK

CH REP

Senectovia Medizinaltechnik AG
In der Luberzen 1,
8902 Urdorf, Switzerland



BASIC UDI-DI: 628758RAZDESIGNINC2004V9

SAFETY PRECAUTIONS

Failure to comply may cause injury or damage!

It is important that the Raz Mobile Shower Commode Chair be properly assembled and that all adjustments be made carefully. Please ensure that the user(s), dealer(s), and attendant(s) have read this manual and thoroughly understood the safe operation of the Raz Shower Chair. Up-to-date manuals are available online at www.razdesigninc.com. For clarification of any section of this manual, contact your distributor or the manufacturer.

Any unauthorized modification/alteration, or misuse of Raz Shower Commode Chairs and accessories is strictly prohibited. Such actions will immediately void any applicable warranty and may result in serious injury, device malfunction, or regulatory non-compliance. Raz Design assumes no liability for any damages, losses, or expenses arising from the use of an unauthorized modified/altered device. The user assumes all responsibility for ensuring the device is used as intended and specified in the official documentation.



MANUFACTURER

Raz Design Inc.
135 Railside Rd. Toronto, ON, Canada, M3A 1B7
877.720.5678 / +1.416.751.5678
info@razdesigninc.com



CHAIR CLASSIFICATION BASED ON MAXIMUM USER WEIGHT	
AT	185 Kg (407 lbs)

SAFETY WARNINGS TO CONSIDER FOR USER PURPOSES

THIS DEVICE IS SUITABLE FOR TYPE A: HIGH USAGE (e.g. INSTITUTIONS) AND SHOULD NEVER BE USED FOR ANY PURPOSE OTHER THAN ORIGINALLY INTENDED

Stability

The casters on all models are equipped with dual-locks. The step-on pedal activates both the roll lock and the swivel lock. ***It is essential that all casters on the shower chair be in an outward position before engaging the locks, for optimal forward, rearward and lateral stability.*** If equipped, disengage the optional directional caster lock before rotating the rear caster to the rearward position and applying the caster's dual-locks.

USERS MUST NOT lean forward while sitting in the Raz Mobile Shower Commode Chair as this may cause the chair to tip forward.

USERS MUST NOT wheel down a ramp without an attendant who can hold onto the chair during the descent.

CASTER LOCKS ARE NOT BRAKES! Never use caster locks to slow down the shower chair when descending inclines as this could cause the chair to tip in the direction of travel.

Lateral Stability

USERS MUST NOT lean over the edge of a Raz Mobile Shower Commode Chair as this could cause the chair to tip.

USERS MUST NOT attempt to pick up objects from the floor by leaning over and reaching – use a reacher or ask for assistance from an attendant.

USERS MUST NOT position the Raz Mobile Shower Commode Chair on a side slope as this could cause it to tip.

Ramps and Other Inclines

Ramps and other surfaces that are not level (such as slopes into wheel-in showers) must be tested with an attendant to ensure that they don't compromise the chair's stability. A qualified healthcare professional should be consulted to assist with this process.

DO NOT push or pull the Raz-AT up or down an incline or ramp that exceeds a 1:12 grade (5° slope).

DO NOT allow any user to be propelled (pushed or pulled) in a Raz-AT except by an attendant.

ALWAYS CHECK THAT THE RAZ-AT SHOWER CHAIR IS STABLE BEFORE IT IS OCCUPIED BY ANY USER AT ANY TIME.



Immersion

The Raz Shower Chair is not designed to be used as a pool chair. Do not immerse the shower chair in whole or in part, in water or any other liquid. Immersion may result in damage to the shower chair.

Chlorine Exposure

Suitable for use in wet areas, but not pools and similarly corrosive environments.

DO NOT store the device near pools because chlorine in the air can cause rust to form on some of the chair's stainless steel components.




IMPORTANT !

CONSULT A HEALTHCARE PROFESSIONAL IF YOU AS A USER EXPERIENCE DISCOMFORT, CHANGES IN MOBILITY, OR DIFFICULTY USING THE DEVICE.

Transfers

The most dangerous part of using any shower chair is the transfer. Since every chair has different stability characteristics, it is essential to carefully review and test the transfer technique to ensure that the procedure is safe. Test transfers should be performed with an attendant who can prevent the chair from tipping or moving during the transfer. If you feel that the transfers cannot be repeatedly performed safely, contact a healthcare professional who is familiar with transfer techniques and options. Individuals who have not learned safe transfer skills must seek assistance during transfers and may require the use of a mechanical lift.

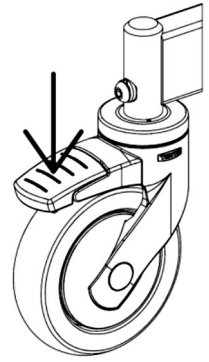

Transferring onto a Raz-AT Shower Chair


ALWAYS lock all four casters, with the front casters positioned forward for maximum chair stability.

Transfers should never be attempted with the shower chair positioned on slippery surfaces. It is recommended that transfers be performed on clean, dry, non-slippery surfaces. Hard surface flooring such as tile, wood, or concrete may not provide sufficient grip to keep locked casters and/or rear wheels from sliding. A fully carpeted surface is optimal. Be aware that area rugs and shower mats can slide on floors and thereby present a hazardous surface.



DO NOT stand on any part of the frame of the Raz-AT Shower Chair.

NEVER use the footplates to assist in transfers. This could cause the chair to tip. The foot supports should be swung to the side or removed entirely during transfers to provide unobstructed access to the shower chair.

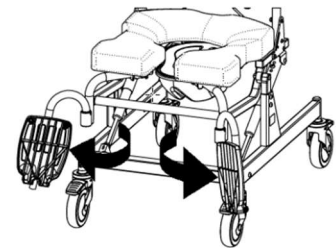

Tilt Function

ALWAYS check the tilt function and ensure both locking gas springs and release cable assemblies are fully operational **BEFORE** the chair is occupied by the user.

A pelvic strap can act as an additional safeguard for the user. A pelvic strap may be ordered as an option with the Raz-AT.

DO NOT attempt to tilt an occupant if the attendant is physically incapable of safely and smoothly operating the tilt function.

NEVER leave the user unattended in a Raz-AT.

IMPORTANT !

USERS SHOULD NEVER BE LEFT UNATTENDED IN A RAZ MOBILE SHOWER COMMODORE CHAIR.


IMPORTANT !

DO NOT LIFT A RAZ MOBILE SHOWER COMMODORE CHAIR AND OCCUPANT BY THE ARM SUPPORTS OR FOOT SUPPORTS!

IMPORTANT !

ALWAYS BE SURE THAT THE SEAT IS PROPERLY INSTALLED AND LATCHED BEFORE A USER IS TRANSFERRED ONTO THE CHAIR. THE REAR SEAT ATTACHMENT BRACKETS MUST BE FULLY HOOKED UNDER THE REAR SEAT SUPPORT TUBES. THE FRONT SEAT ATTACHMENT BRACKETS MUST BE SECURELY LATCHED AROUND THE FRONT SEAT SUPPORT TUBES. BOTH FRONT AND REAR SEAT ATTACHMENT BRACKETS SHOULD BE SECURED IN PLACE BY TIGHTENING THE 8 SCREWS ON THE UNDERSIDE OF THE SEAT.

INSTRUCTIONS FOR THE PROPER REMOVAL AND INSTALLATION OF THE SEAT FOR CLEANING MUST BE PROVIDED TO THE USER AND / OR ATTENDANTS.

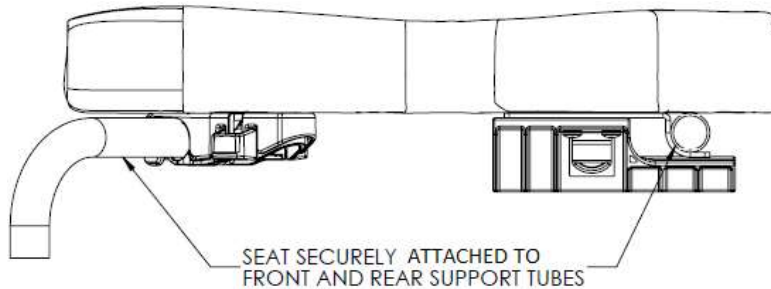

INTENDED USE STATEMENT

INDIVIDUALLY CONFIGURED, MOBILE AND STATIONARY COMMODE CHAIR FOR USE DURING SHOWERING AND TOILETING.

IMPORTANT !

THE RAZ-AT IS INTENDED FOR FOLLOWING USES:

- AS AN AID FOR SHOWERING/BATHING, GOING TO THE TOILET, AND OTHER ACTIVITIES ASSOCIATED WITH PERSONAL CARE AND PERSONAL HYGIENE;
- AS A SUPPORT FOR THE BODY OF THE USER IN A SEATED OR RECLINED POSITION;
- WITH OR WITHOUT THE ASSISTANCE FROM A CAREGIVER;
- OVER A STANDARD TOILET, OR AS A COMMODE WITH THE COMMODE PAN;
- IN INDOOR ENVIRONMENTS ONLY;
- IN BOTH TYPE A, HIGH USAGE (e.g. INSTITUTIONAL) ENVIRONMENTS AND IN-HOME ENVIRONMENTS

THE RAZ-AT DOES NOT PERFORM ANY THERAPEUTIC OR DIAGNOSTIC FUNCTIONS AND IS NOT INTENDED FOR USE FOR ANY THERAPEUTIC OR DIAGNOSTIC PURPOSES. ALL PRODUCTS WITHIN THE RAZ FAMILY ARE NON-STERILE, REUSABLE, NON-INVASIVE, AND NON-IMPLANTABLE.

THE RAZ-AT IS INTENDED TO BE USED BY PEOPLE WITH MOBILITY IMPAIRMENTS, WHO MAY HAVE DIFFICULTY IN STANDING OR KEEPING THEIR BALANCE WHILE COMPLETING ACTIVITIES SUCH AS SHOWERING, TOILETING, OR PERSONAL HYGIENE. TYPICAL USERS HAVE LIMITED ENDURANCE AND POSTURAL CONTROL AND MAY REQUIRE ASSISTANCE FROM A CAREGIVER FOR ACTIVITIES SUCH AS SHOWERING, TOILETING, OR PERSONAL HYGIENE. FOR PRODUCTS WITH RECLINE FUNCTION, USE OF THE RECLINE FUNCTION MAY BE CONTRA-INDICATED WHERE THE USER IS SENSITIVE TO SHEARING FORCES ON SEATED SURFACES WHEN OPENING THE SEAT-TO BACK-ANGLE.


LABELS OR SYMBOLS ON THE PRODUCT

PRODUCT DESIGNATION	RAZ-AT
MANUFACTURER ADDRESS	 Raz Design Inc. 135 Railside Road Toronto, ON Canada M3A 1B7
AUTHORIZED REPRESENTATIVE DETAIL	EC REP UKRP CH REP
PRODUCT IDENTIFIER (PI)	SN RAT-XXXXXX
UDI-DI	UDI 628758003007
MEDICAL DEVICE	MD
EUROPEAN CONFORMITY	
DATE OF MANUFACTURE	
MAXIMUM USER WEIGHT	
READ USER MANUAL	

FRONT SEAT BRACKET INSTALLATION (IF APPLICABLE)



TORONTO, CANADA

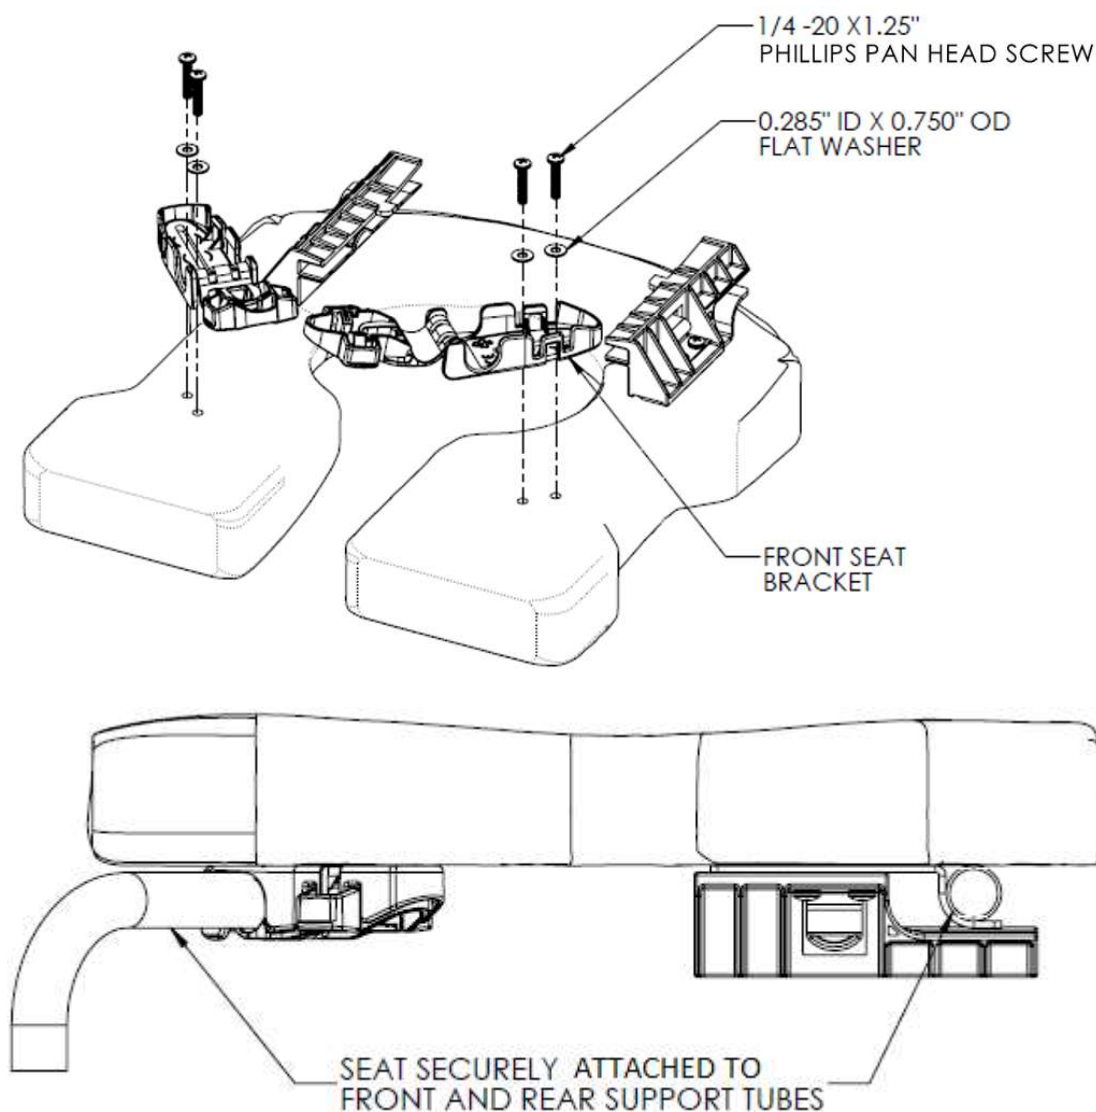

Please refer to the above image for the installation procedure.

Note: Please install the Phillips Pan Head Screws by hand. The use of power tools may cause the bracket to deform.

After installation, ensure the brackets are secured onto the seat. Open and close the brackets to check for proper functionality.


Always be sure that the seat is properly installed and latched. The rear hooks must be fully engaged with the rear seat support tubes and the front brackets must be latched and locked around the front seat support tubes.

USER & DEALER MANUAL TABLE OF CONTENTS

1.0 GENERAL INFORMATION	9
1.1 Raz-AT Mobile Shower Commode Chair Overview	9
1.2 Raz-AT Mobile Shower Commode Chair Specifications	9
2.0 SET-UP: INTENDED FOR DEALER USE ONLY	10
2.1 Back Support	10
2.1.1 Back Support Installation	10
2.1.2 Back Support Angle Adjustment	10
2.1.3 Adjustable-Tension Back Upholstery Adjustment	11
2.2 Caster Installation	11
2.3 Arm Support Adjustment – Adjusta-Back Option Only	11
2.3.1 Arm Support Height Adjustment	11
2.3.2 Arm Support Angle Adjustment	11
2.4 Raz Seats	12
2.4.1 Raz Seat Installation	12
2.4.2 Ischial Pelvic Alignment System (IPAS) – Adjustment	12
2.5 Seat-To-Floor Height Adjustment	13
2.6 Adjustable Foot Supports	14
2.6.1 Foot Support Installation	14
2.6.2 Foot Support Adjustment	14
2.7 Molded Head Support	14
2.7.1 Head Support Installation	14
2.7.2 Head Support Adjustment	14
2.8 DEALER USE ONLY - Fastener Installation	15
3.0 USE AND OPERATION	16
3.1 Tilt Function	16
3.2 Tilt-Assist Pedal	16
3.3 Flip-Up Arm Supports	16
3.4 Adjustable-Tension Back Upholstery	17
3.5 Raz Seats	17
3.6 Adjustable Foot Supports (Footrests)	17
3.7 Molded Head Support (Headrest)	18
3.8 Commode Pan	18
4.0 CLEANING AND MAINTENANCE	19
4.1 Cleaning After Each Use	19
4.1.1 Commode Pan	19
4.1.2 Seat	19
4.2 Cleaning As Needed	19
4.2.1 Adjustable-Tension Back Upholstery	19
4.2.2 Frame, Arm Supports, Adjustable Foot Supports, and Other Components	19
4.3 Suggested Cleaning Products	19
5.0 INCIDENT REPORTING	20
6.0 LIMITED WARRANTY	20
7.0 CONTACTS	21

1.0 GENERAL INFORMATION

1.1 Raz-AT Mobile Shower Commode Chair Overview

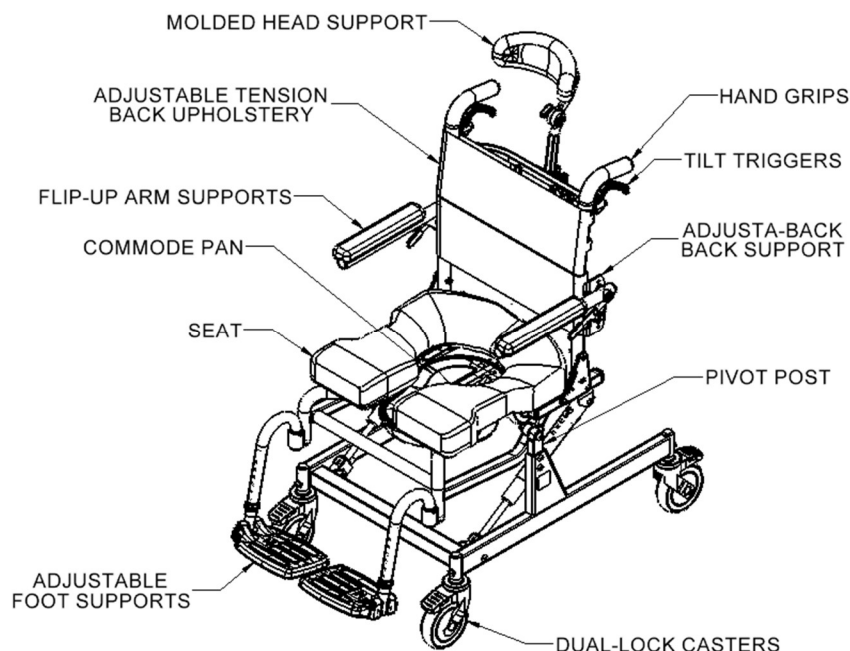

1.2 Raz-AT Mobile Shower Commode Chair Specifications

SPECIFICATIONS	Raz-AT
WEIGHT CAPACITY	185 kg (407 lbs)
FRAME WIDTH seat and back frame	46 cm (18")
OVERALL WIDTH	58 cm (22.75")
OVERALL LENGTH at 0° tilt, with foot supports	102 cm (40")
OVERALL LENGTH at 40° tilt, with foot supports	139 cm (54.75")
SEAT WIDTH commode seat	46 cm (18")
SEAT DEPTH front of the back post to the front of the seat	41-46 cm (16"-18"), 48-53 cm (19"-21")
CLEARANCE WIDTH	40 cm (15.75")
CLEARANCE HEIGHT with pan brackets	43-53 cm (17"-21")
CLEARANCE HEIGHT without pan brackets	45-55 cm (17.75"-21.75")
ARM SUPPORT (ARMREST) HEIGHT ABOVE SEAT with Adjusta-Back	44 cm (17") high back: 17-24 cm (6.5"-9.5") 51, 61 cm (20", 24") high back: 19-27 cm (7.5"-10.5") in 1.25 cm (½") increments
SEAT-TO-FLOOR HEIGHT	55-65 cm (21.5"-25.5") in 2.5 cm (1") increments
PRODUCT WEIGHT with foot supports	28 kg (61 lbs)
FRAME AND HARDWARE MATERIAL	Stainless Steel (Lifetime warranty against corrosion)
MINIMUM TURNING CIRCLE	109 cm (43")

2.0 SET-UP: INTENDED FOR DEALER USE ONLY

IMPORTANT NOTE: If the threads are not lubricated, cold-welding of fasteners can occur.

- Apply a lubricant (liquid detergent, soap, lip balm, wax, etc.) to the threads before tightening the fasteners to reduce the possibility of cold welding.
- Do not overtighten fasteners.

IMPORTANT !

ADJUSTMENTS SHOULD NEVER BE ATTEMPTED WITH THE USER IN THE CHAIR.

2.1 Back Support

2.1.1 Back Support Installation


Tools required: 5/32" hex key, 7/16" wrench

1. Remove the shower chair from the shipping carton.
 2. Lift the back support upright to align the holes.
 3. Insert a button head cap screw through one of the two holes on the back support plate and then push through the back post.
- NOTE: Select the rear hole for a 90° back support angle or the front hole for a 97° back support angle.


TIP: Temporarily position the back support upright by inserting a Phillips screwdriver through one plate and back post.

4. Attach the curved washer and locknut as shown below.
5. Tighten the assembly with the hex key and wrench until the end of the screw extends 1 or 2 threads beyond the locknut.
6. Repeat steps 3 to 5 for the other back post.

Note: Re-lubricate fasteners prior to tightening.

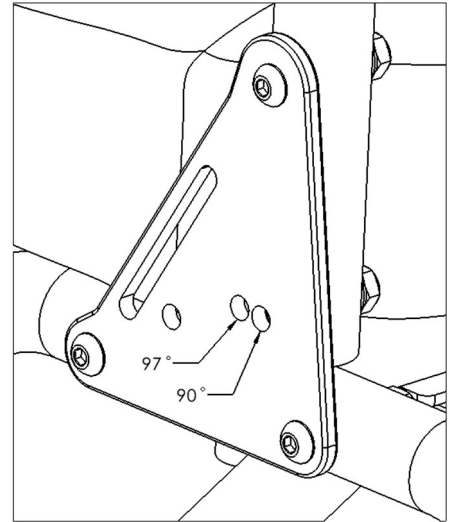

TOP VIEW OF THE BACK SUPPORT INSTALLATION

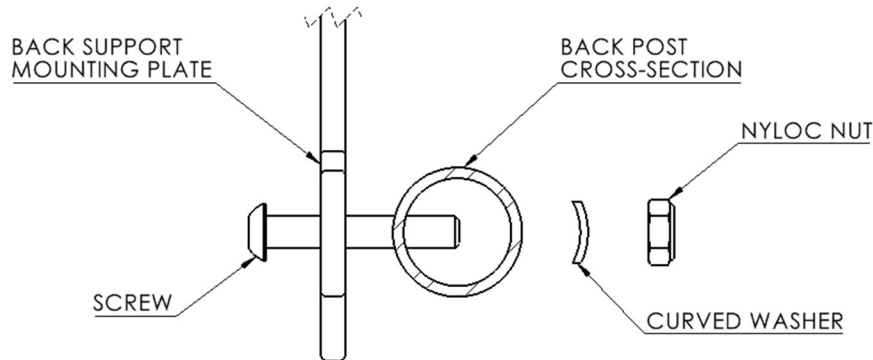


2.1.2 Back Support Angle Adjustment

Tools required: 5/32" hex key, 7/16" wrench

1. Loosen (do not remove) the top screws and locknuts and attaching the back support mounting plate to the back posts.
2. Remove the lower screws and washers from both sides.
3. Rotate the back support to align the back post hole to one of the 2 positions on the back support mounting plates.

NOTE: Select the rear hole for a 90° back support angle or the front hole for a 97° back support angle.

4. With the back support in place, insert the screws through the selected holes on the back support mounting plates.
5. Fasten the screws with curved washers and locknuts.
6. Tighten the assembly with the tools.

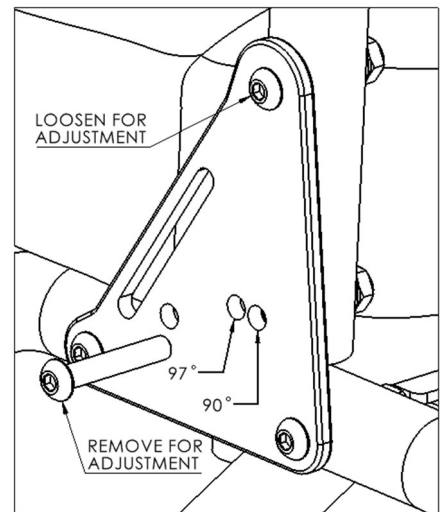

2.1.3 Adjustable-Tension Back Upholstery Adjustment


In order to adjust the back upholstery, each strap can be tightened or loosened in the buckles to achieve a wide range of positions. For example, the second and third straps from the bottom can be tightened to create more pronounced support in the lumbar area of the back.

2.2 Caster Installation

The Raz-AT chairs are shipped with casters not installed. Please follow the instructions below for caster installation.

Tool required: 5mm hex key

1. Remove the Raz-AT from the shipping carton.
2. Insert caster stem into caster housing on the base frame.
3. Align the hole in the caster stem with the hole in the caster housing.
TIP: Apply the caster lock to facilitate aligning the hole
4. Insert the M8 button-head screw into the hole on the caster housing.
- NOTE: Ensure each M8 screw has medium-strength thread locker solution on its threads before using.*
5. Thread the M8 screw through the caster housing and into the caster stem.
6. Continue to thread the M8 screw until it is tight.
7. Repeat steps 1 to 5 until all four casters are secured in place.

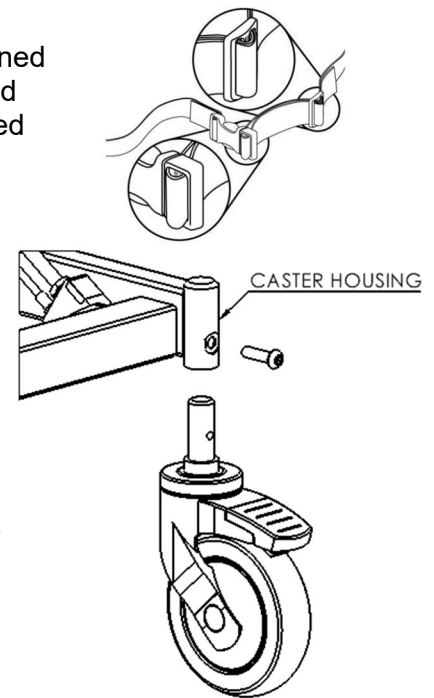

2.3 Arm Support Adjustment – Adjusta-Back Option Only

Tools required differ by hardware, make sure the correct tools are selected for secure installation. Frame with the identifier hole is Metric.

- for Imperial 3/8" hardware: 7/32" hex key, 9/16" wrench;
- for Metric M8 hardware: 5mm hex key, 13mm wrench

2.3.1 Arm Support Height Adjustment


The arm supports are adjustable in height within a 3" range, in 1/2" increments *on the Adjusta-Back Option only*.

1. Loosen and remove the lower locknut.
2. Loosen and remove the upper locknut.
3. Keeping the arm support and arm support pivot plate assembly together, move the unit up or down on the arm support weldment depending on the user's needs.
4. Reinstall the locknut onto the upper screw.
5. Reinstall the locknut onto the lower screw.
6. Tighten screws and locknuts at the upper and lower.
7. Repeat steps 1 to 6 for the other arm support.

2.3.2 Arm Support Angle Adjustment

The arm support angle can be adjusted up 5° or down 5° if the back support angle is adjusted from the 90° factory position.


1. Loosen and remove the screw, washer and locknut on the bottom of the arm support pivot plate.
2. Keeping the upper screw in place, rotate the arm support assembly until the preferred position is reached by aligning one of the 3 holes (arranged in a triangle) on the arm support pivot plate with the holes on the arm support weldment.
3. Insert the screw into the preferred position on the arm support pivot plate and attach the locknut.
4. Tighten the screw and locknut.
5. Repeat steps 1 to 4 for the other arm support.

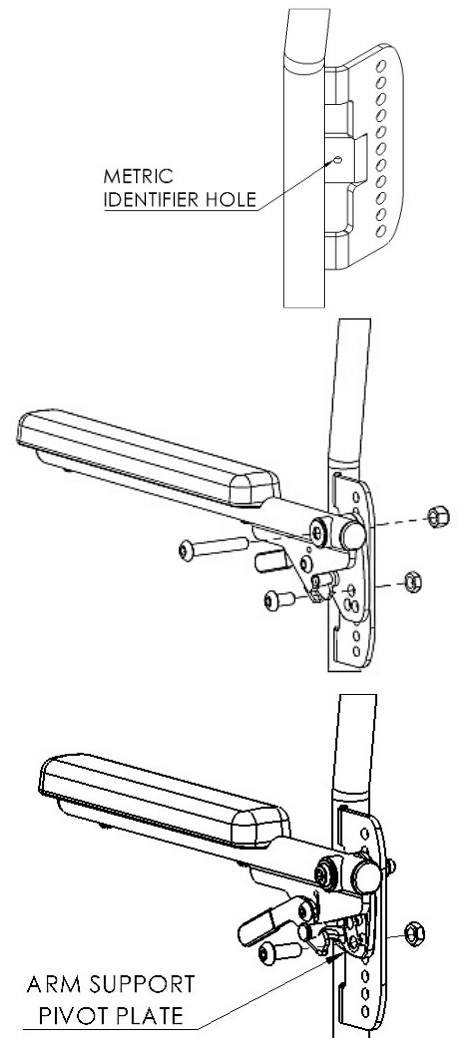

2.4 Raz Seats

2.4.1 Raz Seat Installation

1. Ensure that the front brackets are in the open position.
To open the front brackets, simply squeeze the tabs or the hinged portion of the bracket.
2. Slide the rear of the seat over the rear cross tubes as the front of the seat is lowered onto the frame. Ensure that the rear seat brackets hook below the cross tubes.
3. Continue lowering the front of the seat until the front seat brackets nestle onto the front seat support tubes.
4. Secure the seat in place by closing the front seat brackets.
To close the seat bracket, snap the clamp back onto its other half around the front support tubes.
5. Reverse steps 1 to 4 to remove the seat from the frame.

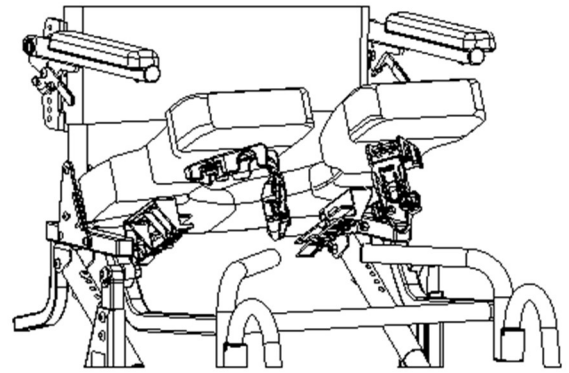

*Please see page 4 for additional information.

2.4.2 Ischial Pelvic Alignment System (IPAS) – Adjustment

The seat has approximately 5 cm (2") of fore/aft adjustment, allowing optimal positioning of the seat aperture around the user's Ischial Tuberosities.


Tool Required: #2 Phillips screwdriver

1. Release the seat by squeezing the tabs to open the front seat brackets.
2. Lift the front of the seat and pull upward and then forward to remove the seat from the chair.
3. Loosen (*but do not remove*) the eight screws attaching the front seat brackets and rear seat brackets to the underside of the seat.

Note: For clarity, the rear seat brackets are shown below without commode pan brackets.

4. Place the seat on the frame and close the front seat brackets around the front seat support tubes.
5. Slide/wiggle the seat to the desired position.
6. Ensure rear seat brackets are firmly positioned against the rear seat support tube.
7. Tighten all eight screws attaching the front and rear seat brackets to the seat to prevent further movement of the seat.

Note: Ensure the front and rear seat brackets are securely latched around the front and rear seat support tubes before allowing a user to transfer into the chair.



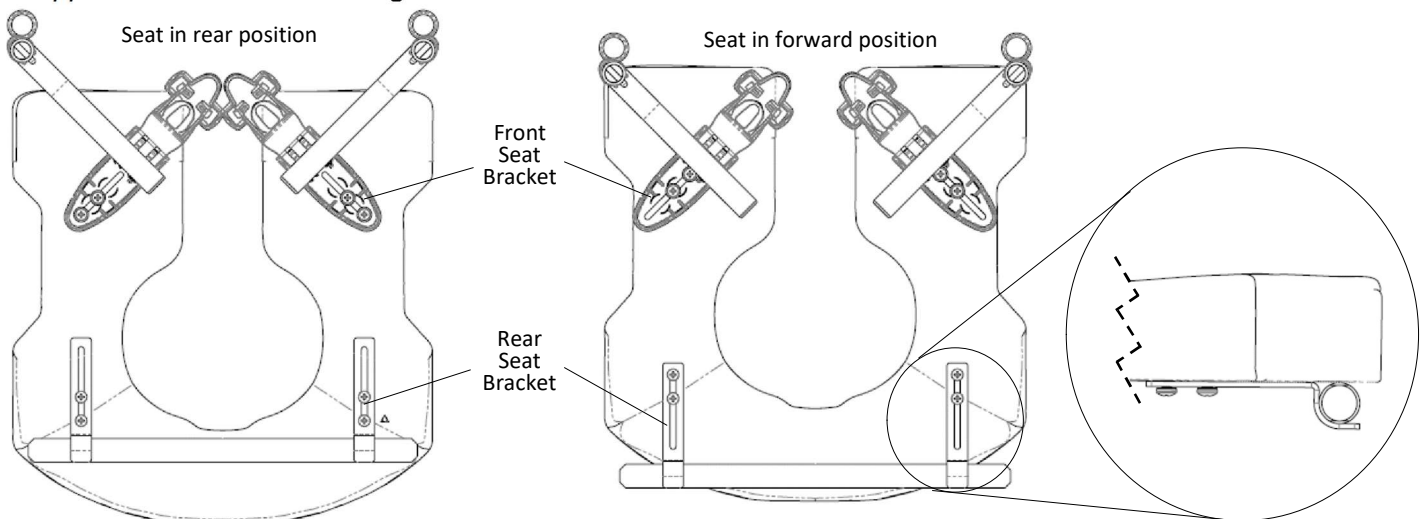


2.5 Seat-To-Floor Height Adjustment

To change the seat-to-floor height on a Raz-AT model, adjust the pivot post heights on both sides of the chair.

Tools required: 5mm hex key, 13mm socket wrench

1. Ensure the chair is out of tilt by squeezing both tilt triggers.
2. Remove the foot supports if they are installed.
3. On a soft and clean surface (e.g. carpeted surface, flattened packaging box), carefully tip the chair forward as in the drawing below.

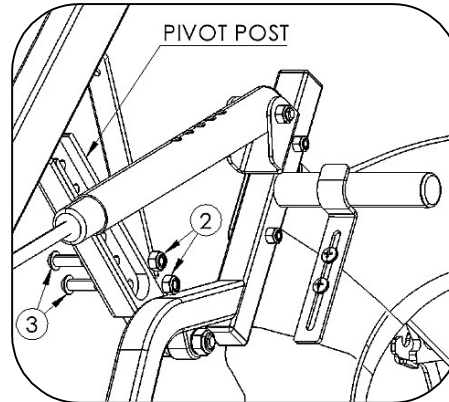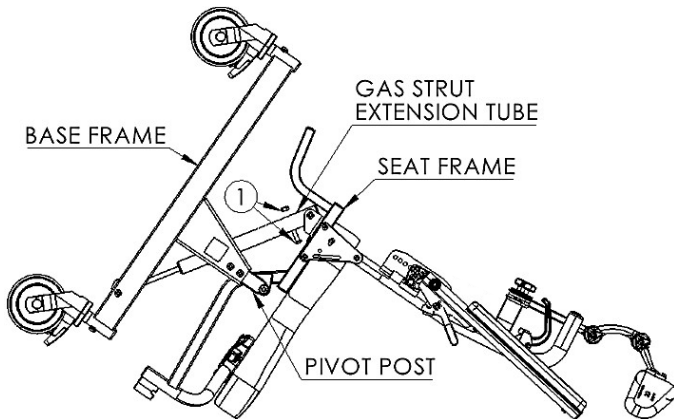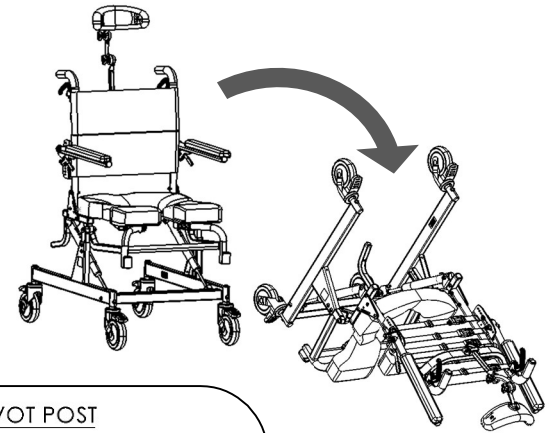




4. Remove the screws and locknuts ① from both gas strut extension tubes.
5. Remove the locknuts ② from both pivot posts. If needed, pivot the base frame for better access to the locknuts.
6. Remove the screws ③ from both sides.

Tip: Slightly lift the base frame to relieve the pressure on the screws during removal or use a hex key to back out the screws.

7. Move the base frame along the pivot posts to the desired seat-to-floor height.
8. Align the pivot posts' holes to the base frame's holes.
9. Insert the screws ③ into the aligned holes on both sides.

Tip: Insert one screw on each side first rather than inserting both screws on one side before the other side.


10. Attach the locknuts ②.
11. Level the seat frame to be parallel with the base frame, and align the eyelet of each gas strut to the nearest hole of the gas strut extension tube.
12. Install the screws through the aligned holes and attach the locknuts ①. The screws must be inserted through the gas strut extension tube and the eyelet of the gas strut as shown.
13. Ensure all hardware is installed securely before raising the chair to an upright position.

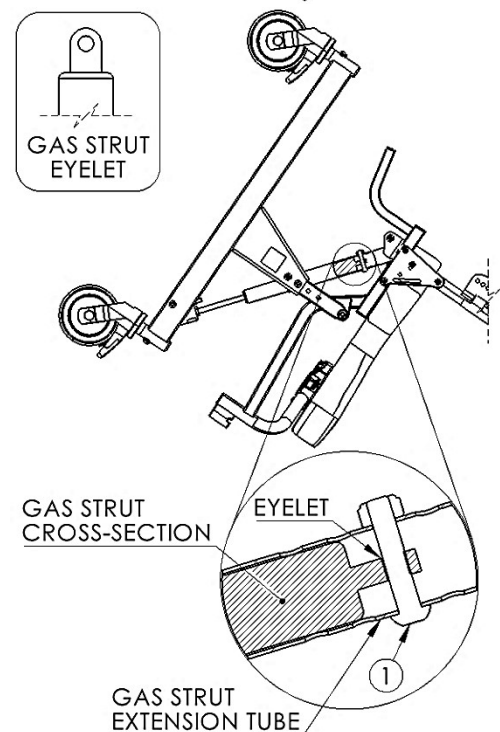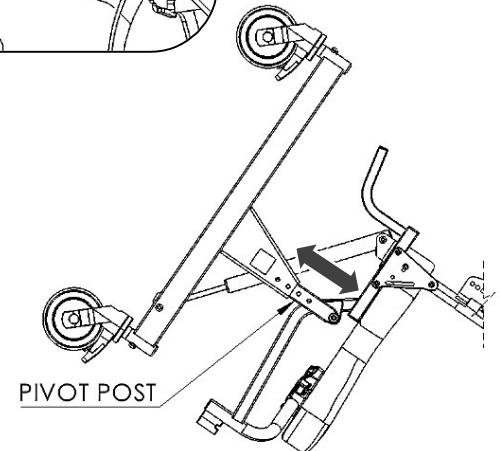

2.6 Adjustable Foot Supports


2.6.1 Foot Support Installation

1. Remove the foot supports from the inner accessory box.
2. Place the foot support hanger tubes into the receivers, welded at the front of the chair frame. *If the support tubes are directed forward, the pins on the tubes will engage with grooves in the receivers and lock in place.*

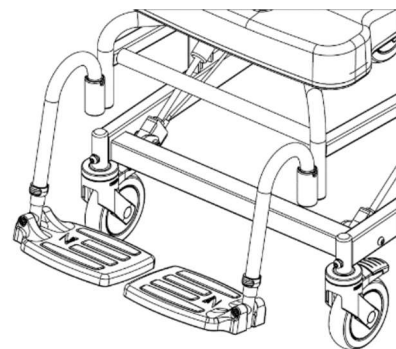

2.6.2 Foot Support Adjustment

1. Remove a plastic snap-pin from one foot support hanger tube.
2. Adjust the footplate extension tube vertically to achieve the desired height in the foot support hanger tube.
3. Insert the snap-pin through the foot support hanger and the extension tubes. Ensure that the snap-pin is completely through the tube and that the green plastic clip is snapped securely around the outside of the hanger tube.
4. Repeat steps 1 to 3 for the other footplate

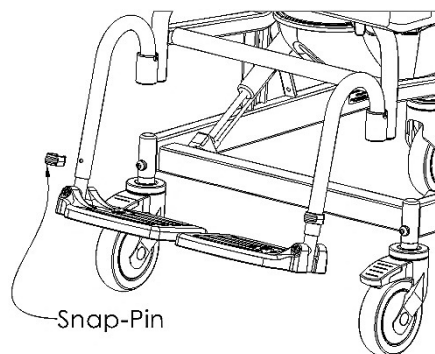


2.7 Molded Head Support

A molded head support is included with all Raz-AT Shower Chairs. It is shaped to cradle the head comfortably and is easy to clean. The head support can be adjusted indefinitely forward and backward within a 5" range and vertically within a 5½" range.

2.7.1 Head Support Installation

1. Remove the head support assembly from the inner accessory box.
2. Insert the square tube of the head support assembly into the receiver on the back support while ensuring the molded pad is facing forward.
3. Unfold the head support by loosening the Tri-lobes.
4. Adjust the angle and height to the user's preference.
5. Tighten the Tri-lobes fully to secure the angle and height of the molded head support.

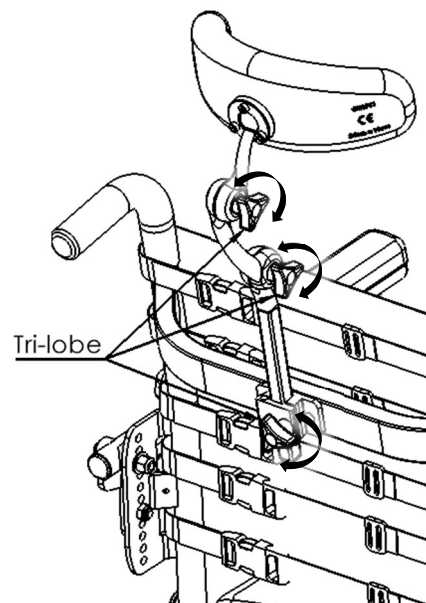

2.7.2 Head Support Adjustment


To adjust the position of the head support:

1. Loosen the Tri-lobes on the head support assembly.
2. Adjust the angle and height to the user's preference.
3. Tighten the Tri-lobes to fully secure the head support position.

To adjust the angle of the head support pad:


Tool required: 4mm hex key

1. Loosen (do not remove) the three screws on the back of the molded head support.
2. Rotate the head support pad around the end of the head support mounting bar to suit the user's needs.
3. Tighten the screws to secure the position of the pad.
4. Ensure that all knobs and screws are tightened securely for the user's safety.

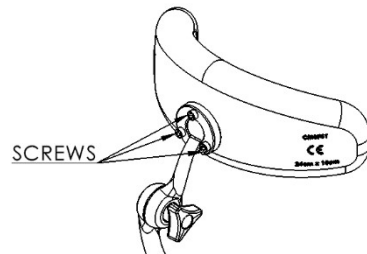

2.8 DEALER USE ONLY - Fastener Installation

All fasteners should be installed securely. Locknuts removed for any reason may need to be replaced rather than re-used. Check the performance of nyloc nuts when re-attaching to the screw. There should be significant detectable resistance when tightening. If not, replace the nyloc nut with a new one. It is advisable to check annually that all fasteners are secure.

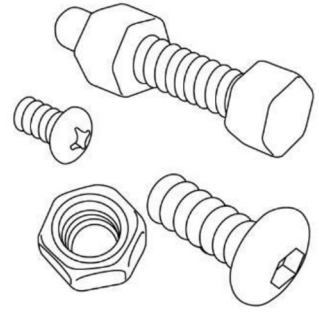

IMPORTANT !


INCREASING THE SEAT HEIGHT AND THE BACK SUPPORT ANGLE WILL DECREASE REARWARD STABILITY. IT IS ESSENTIAL THAT A STABILITY CHECK BE PERFORMED AFTER ANY OF THESE ADJUSTMENTS ARE MADE.

3.0 USE AND OPERATION

3.1 Tilt Function

The Raz-AT Shower Commode tilts up to 40° to provide comfort and relieve pressure for the user. Two gas spring struts facilitate this tilting action, making the tilt smooth for the user and the attendant. The attendant must squeeze both tilt triggers to tilt the chair to the desired angle. To lock the chair in place, the attendant can release the triggers. Directly after purchase, the triggers and springs may seem stiff. This stiffness is normal and diminishes with use. Using the tilt-assist pedal will help to tilt the seat frame back. The tilt function must only take place when the casters are locked.

NOTE: When the chair is mounted at the lowest height setting the maximum potential tilt angle is 40°. The higher the chair is set, the fewer degrees the chair can be tilted back. (With a seat-to-floor height of 25" the chair can be tilted back 36°).

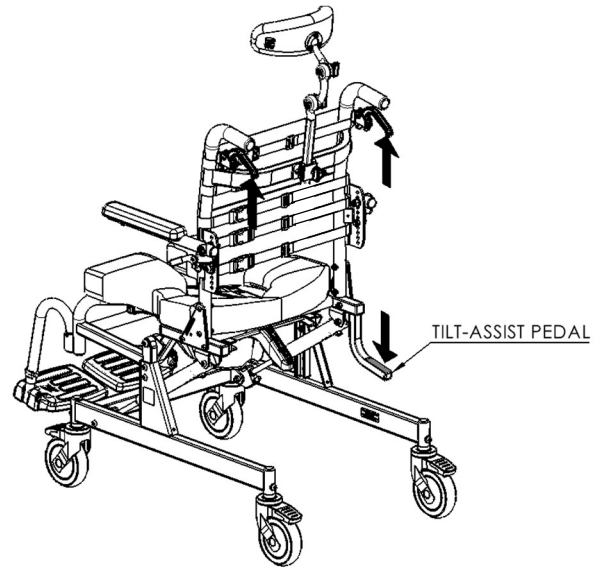

IMPORTANT !


DO NOT ATTEMPT TO TILT A RAZ SHOWER CHAIR IF THE ATTENDANT IS PHYSICALLY INCAPABLE OF SAFELY AND SMOOTHLY OPERATING THE TILT MECHANISM WITH A USER OCCUPYING THE CHAIR. ANY ATTENDANT MUST BE FAMILIAR WITH PROPER TILTING TECHNIQUES PRIOR TO ASSISTING A USER IN THE SHOWER COMMODE. A PELVIC STRAP IS RECOMMENDED FOR ANY USER AS AN EXTRA SAFETY PRECAUTION.

IMPORTANT !

NEVER ATTEMPT TO CHANGE THE SEAT HEIGHT WITHOUT THE HELP OF A QUALIFIED DEALER. HIGHER SEAT POSITIONS WILL REDUCE THE CHAIR'S STABILITY AND MAY RESULT IN TIPPING AND INJURY.


3.2 Tilt-Assist Pedal

A Tilt-Assist Pedal is standard on the Raz-AT Shower Chair to facilitate tilting the chair for attendants.

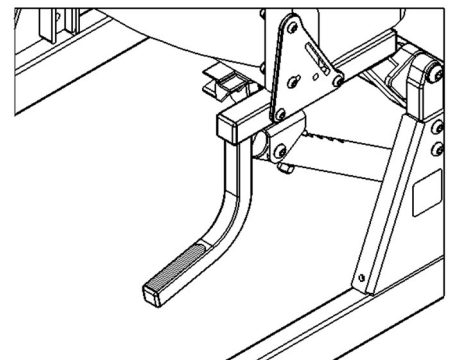

3.3 Flip-Up Arm Supports

The Adjusta-Back is adjustable in angle and has arm supports that can be adjusted in height and angle. The arm supports can flip up to allow for ease of transfer, and lock automatically (if the optional lock is included) when flipped down.

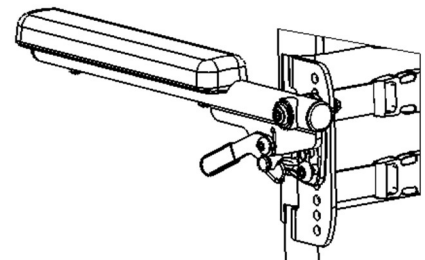


3.4 Adjustable-Tension Back Upholstery

The Adjusta-Back back supports come with an Adjustable-Tension Back Upholstery that provides trunk support for optimal positioning and comfort. The upholstery is removable for machine washing and available in the 15" (4 straps), 17" (5 straps), 20" (6 straps), and 24" (7 straps) heights in accordance with the back height selected for the chair.


To install Adjustable-Tension Back Upholstery on a 17" high Adjusta-Back:

1. Place the fabric against the front of the back support canes making sure that when wrapped around, the clips on the straps face away from the fabric and the loops point downwards.
2. The highest strap (1) is positioned above the crossbar.
3. Second (2) and third (3) straps are positioned between the crossbar and back support mounting plates. A 15" high back will only have a single strap at this location.
4. The fourth (4) and fifth (5) straps are fed through the slots in the arm support mounting plates.
5. A 20" high back includes a sixth strap, which should be positioned below the arm support mounting plates.
6. Adjust all of the straps to meet the user's needs.

NOTE: For the 24" Adjusta-Back, the two highest straps should be positioned above the back support crossbar. The other five straps are located the same as the 20" Adjusta-Back.

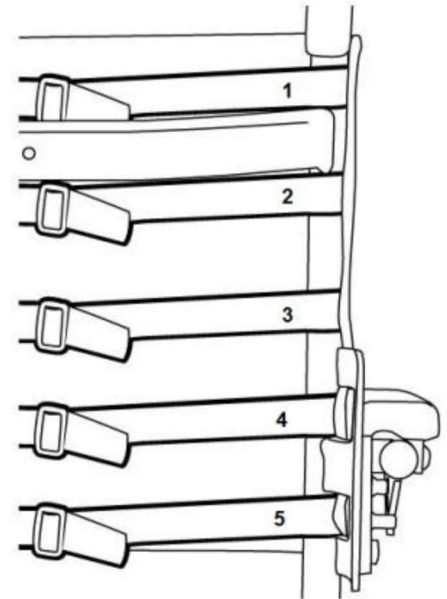

In order to adjust the back upholstery of the back support, each strap can be tightened or loosened to achieve a wide range of positions. For example, the second and third straps from the bottom can be tightened to create more pronounced support in the lumbar area of the back.

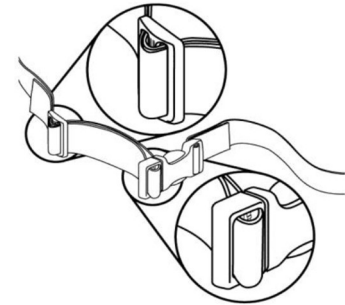


To remove the Adjustable-Tension Back Upholstery, release the buckles on the straps.

3.5 Raz Seats

To install a Raz Seat:

1. Ensure that the front brackets are in the open position. To open the front brackets, simply squeeze the tabs on the hinged portion of the bracket.
2. Slide the rear of the seat over the rear cross tubes as the front of the seat is lowered onto the frame. Check to make sure that the rear seat brackets hook below the cross tubes.
3. Continue lowering the front of the seat until the front seat brackets nestle onto the front seat support tubes.
4. Secure the seat in place by closing the front seat brackets. To close the seat bracket, snap the clamp back onto its other half around the front support tubes.
5. Reverse steps 1 to 4 to remove the seat from the frame.

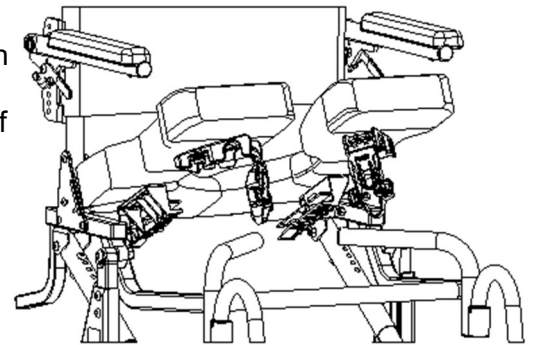


*Please see page 4 for additional information.

IMPORTANT !

FRONT AND REAR OPEN (FAR) SEATS MUST HAVE CLAMPS INSTALLED AND PROPERLY ADJUSTED ON THE SEAT FRAME.

IPAS ADJUSTMENT OF FAR SEAT MUST BE FOLLOWED BY PROPER ADJUSTMENT OF CLAMPS BY A QUALIFIED RAZ DEALER. REFER TO THE PROVIDED INSTRUCTION SHEET OR SECTION 2.4.3 FOR MORE DETAIL.

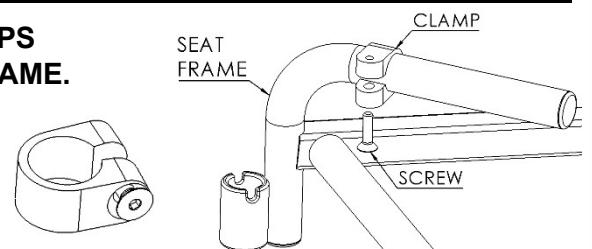

1. Place the footrest hanger tubes into the footrest receivers.
2. If the hanger tubes are aligned forward, the pins on the tubes will engage with grooves in the receivers and lock in place.


To adjust the length of the Adjustable Footrests:

1. Remove the snap-pin from one footrest hanger tube.
2. Reposition the footplate to a length suitable for the user.
3. Insert the snap-pin through the footrest hanger tube and through the inner tube.

To rotate the Adjustable Footrests:

1. Lift the footrest hanger tubes to disengage the pins.
2. Rotate the footrests outward or inward.

To remove the Adjustable Footrests, lift the footrests out of the receiving sleeves on the frame.

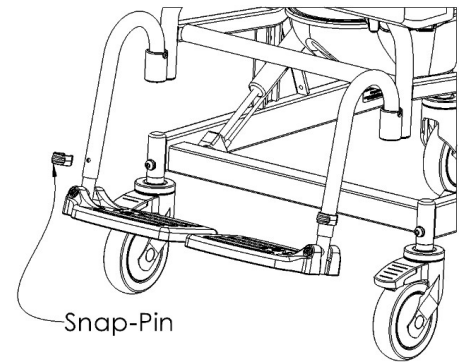


3.7 Molded Head Support (Headrest)

A molded headrest is included with all Raz-AT Shower Chairs. It is shaped to the head comfortably and is easy to clean. The headrest can be adjusted in forward and backward within a 5" range and vertically within a 5½" range.

To adjust the molded headrest:


1. Loosen the Tri-lobes on the molded headrest assembly.
2. Adjust the angle and height to the user's preference.
3. Tighten the Tri-lobes fully to secure the angle and height of the molded headrest.
4. Ensure that all Tri-lobes are tightened securely for the user's safety.

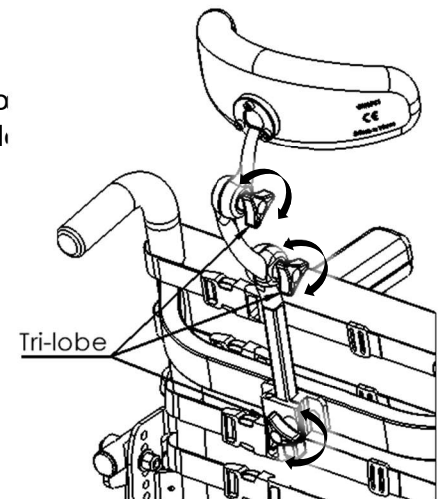

3.8 Commode Pan

The Raz Commode Pan is designed with an elongated shape that fits directly under the seat to minimize backsplash. A unique splash-reduction ridge is located at the center of the pan. The high gloss surface facilitates cleaning and rinsing, while the pouring spout and handle facilitate emptying. Removal of the Commode Pan is achieved by sliding the pan rearward.


NOTE: When re-inserting the pan, ensure that the pan is guided into the green plastic brackets and pushed forward until it hits the stops.

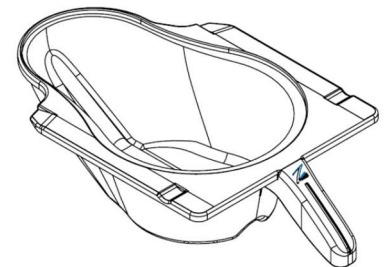

3.9 Casters

Each Raz Shower Chair caster is equipped with a dual-lock feature, which stops the caster from swiveling and rolling simultaneously. To engage the dual-lock, step on the end of the caster brake lever until it latches in the "on" position. To deactivate the dual-lock, step on the raised end of the lever until it releases.

ALWAYS release the directional lock (if applicable) and swivel all four casters to their outward position for maximum stability before transferring or tilting a user.

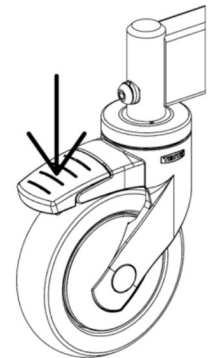

IMPORTANT !

A QUALIFIED RAZ DEALER SHOULD BE CONTACTED TO CHECK ALL FASTENERS, CASTERS, HARDWARE, AND ALL OTHER MOVING COMPONENTS AT LEAST ONCE PER YEAR.

4.0 CLEANING AND MAINTENANCE

4.1 Cleaning After Each Use

4.1.1 Commode Pan

1. Remove the commode pan and empty the contents.
2. Wash the pan with a multi-purpose disinfectant cleaning solution. Use a soft brush if needed.
3. Rinse well before storage or re-use.

NOTE: A soapy hot water wash followed by a disinfectant spray can be substituted for a multi-purpose disinfecting cleaning solution.

4.1.2 Seat

1. Spray with a multi-purpose disinfectant cleaner and scrub with a soft brush as required.
2. Rinse with a water spray before storage or re-use.
DO NOT IMMERSE the seat in water or cleaning solutions.
3. For a more thorough cleaning, remove the seat from the shower chair to allow better access to the seat's underside and around the seat's opening.

4.2 Cleaning As Needed

4.2.1 Adjustable-Tension Back Upholstery

1. Remove the plastic buckles and tri-glides from the back upholstery straps, paying attention to how the straps are wound through each component as they are removed.
2. Remove the back upholstery from the back frame and machine wash with a mild detergent in warm water on a normal or gentle wash cycle. Include other strap accessories such as the H-strap, and pelvic and chest positioning straps.
3. Install the back upholstery and other positioning accessories on the chair and allow it to dry.
DO NOT dry the back upholstery in a clothes dryer or damage to the upholstery may occur.
4. Assemble all plastic buckles and tri-glides onto straps.
5. Adjust the straps to the desired tension.

4.2.2 Frame, Arm Supports, Adjustable Foot Supports, and Other Components

1. Spray the frame and components with a multi-purpose disinfectant cleaner, scrub with a soft brush, and rinse with water.
2. If necessary, spray the frame and components with a diluted (10 parts water to 1 part solution) calcium/lime remover (such as CLR), scrub with a soft brush, and rinse thoroughly with water.
DO NOT mix a calcium/lime removal solution with any other liquid or toxic fumes may occur.
DO NOT use chlorine bleach on any Raz components.

It is recommended to the user that a qualified Raz dealer check all fasteners and subassemblies to see if there is cause for concern regarding the shower chair's performance.

Several times each year the shower chair and its components should be wiped down with a diluted calcium/lime removal solution to reduce deposits, followed by a hot water rinse.

To reduce the risk of mildew buildup, the entire chair should be wiped down with a soft dry cloth after the final rinse and before storage or use.

4.3 Suggested Cleaning Products

Task	Recommended Products
General Cleaning	Antibacterial Detergent
Tuberculocidal Surface Cleaner Intermediate Level Disinfectant	Oxiver TB (Virox Technologies Inc.) SepteFX 7D-11 (Titan Worldwide Inc.)
Calcium and Lime Deterrent	CLR

IMPORTANT !

DO NOT USE ABRASIVE SCRUBBING POWDERS OR SCOURING PADS ON THE RAZ SHOWER COMMODE CHAIR.

DO NOT SUBMERGE THE RAZ SHOWER CHAIR IN WATER.

RINSE THOROUGHLY AFTER CLEANING TO ENSURE ANY SOAP OR DETERGENT RESIDUE IS REMOVED.

DO NOT USE CLEANING PRODUCTS WITHOUT CONSULTING THE PRODUCTS' INSTRUCTIONS AND TAKING APPROPRIATE PRECAUTIONS FOR HUMAN EXPOSURE TO CHEMICALS.

5.0 INCIDENT REPORTING

IMPORTANT !

If any serious incident occurs in relation to this device, meaning any event that has led, or could lead, to death, serious injury, or serious deterioration in health, it must be reported without delay to:

- **The manufacturer (contact details provided in this manual), and**
- **The competent authority or appropriate regulatory authority in the country where the user or patient is located.**

6.0 LIMITED WARRANTY

This warranty is extended only to the original purchaser/user for Raz Mobile Shower Commode Chairs that have been purchased from a qualified Raz dealer.

This warranty gives you specific legal rights, but you may have additional legal rights depending on your region and country.

This warranty shall be extended to comply with state/provincial laws and requirements.

With regards to the original purchaser/user only, Raz Design warrants its base and back frame components to be free of defects in materials and workmanship for a period of two (2) years from the date of purchase. All other components on the Raz Mobile Shower Commode Chair are covered for a period of one (1) year and are subject to normal wear and tear exclusions. If within such warranty period any such product shall be proven to be defective, the part will be repaired or replaced, at Raz Design's discretion. This warranty does not include any labor or shipping charges incurred in replacement, part installation, or repair of any such product.

For warranty service, please contact the dealer from whom you purchased your Raz Mobile Shower Commode Chair. In the event that you do not receive satisfactory warranty service, please contact Raz Design directly using the contact information located at either the beginning or the end of this manual. In your correspondence, please provide your dealer's name and address, the product type, the date of purchase, and the chair's serial number (on a grey label located on the chair frame), as well as the nature of the product issue. Do not return products to the manufacturer without prior authorization.

Limitations and Exclusions:

The foregoing warranty shall not apply to serial numbered products if the serial number has been removed or defaced, and to products subjected to negligence or an accident. Improper operation, maintenance, or storage may void the warranty coverage on the Raz Mobile Shower Commode Chair.

The warranty does not apply to products modified without Raz Design's express written consent. This includes, but is not limited to, modification through the use of unauthorized parts or attachments, products damaged by reason of repairs made to any component by an individual or individuals who are not employed by a qualified Raz dealer, or to a product damaged by circumstances beyond Raz Design's control. Only Raz Design will have the authority to determine whether or not the circumstances are eligible for warranty coverage. The warranty will not apply to problems arising from normal wear or failure to adhere to the instructions contained in this manual.

The foregoing warranty is exclusive and in lieu of any other warranties, whether express or implied, including the implied warranties of merchantability and fitness for a particular purpose. The sole remedy for violations of any warranty whatsoever will be limited to the repair or replacement of the defective product in compliance with the terms contained in this document.

The application of any implied warranty shall not extend beyond the duration of the express warranty provided herein. Raz Design will not be liable for any consequential or incidental damages to part or whole of a Raz Mobile Shower Commode Chair.

Raz Design Inc. frame and hardware material are made of stainless steel for which we offer a lifetime warranty against corrosion. Please be advised this lifetime warranty is only extended to the original purchaser/user of Raz Shower Chairs that have been purchased from a qualified Raz dealer. Failure to comply with proper cleaning instructions may cause corrosion to the frame thereby voiding this warranty. Additionally, all claims of corrosion are subject to review and a request may be made for the return of the device in question, for a thorough examination, before a replacement order can be processed.

7.0 CONTACTS

It is important that the Raz Mobile Shower Commode Chair be properly assembled and all adjustments be made carefully. Up-to-date manuals can be downloaded from www.razdesigninc.com. For clarification of any section of this manual, contact your distributor or the manufacturer.



MANUFACTURER

Raz Design Inc.
135 Railside Rd. Toronto, ON, Canada, M3A 1B7
877.720.5678 / +1.416.751.5678
info@razdesigninc.com



IMPORTANT !

PRODUCTS THAT CAN NO LONGER BE USED ARE TO BE DISPOSED OF SEPARATELY FROM HOUSEHOLD WASTE. THIS MUST BE DONE ACCORDING TO THE LOCAL AND NATIONAL REGULATIONS FOR ENVIRONMENTAL PROTECTION AND RAW MATERIAL RECYCLING. PLEASE LOOK AT YOUR LOCAL GOVERNMENT WEBSITE FOR FURTHER INFORMATION ON THE CORRECT DISPOSAL PROCESS.

IF IT IS EVER FELT THAT ANY ASPECT OF THE RAZ SHOWER CHAIR IS IN NEED OF MAINTENANCE, CONTACT YOUR DEALER. ANY PROBLEMS THAT COULD AFFECT THE SAFE USAGE OF THE CHAIR MUST BE ATTENDED TO IMMEDIATELY. THE DEALER THAT PROVIDED THE SHOWER CHAIR MUST BE CONTACTED SO THAT REPAIRS CAN BE MADE PRIOR TO RESUMING THE USE OF THE CHAIR. IT MUST BE MADE CLEAR TO THE DEALER THAT THE SHOWER CHAIR IS IN NEED OF MAINTENANCE AND IS UNAVAILABLE FOR USE UNTIL REPAIRS HAVE BEEN UNDERTAKEN AND ALL PROBLEMS RESOLVED.

IF FOR ANY REASON, YOUR DEALER DOES NOT RESPOND TO YOUR SATISFACTION, PLEASE CONTACT RAZ DESIGN:

BY EMAIL	info@razdesigninc.com
BY PHONE	877.720.5678 (North America) +1.416.751.5678 (Rest of World)